


-15kV TOF: -9245 v  
 -3.6kV MCP: -3364 v  
 -2.4kV MCP: -1774 v  
 Input Cur: 326 ma  
 RPA max: 238 v  
 Mirror max: 238 v

Tue Nov 14 10:19:14 2006

## TIDE Direct Events

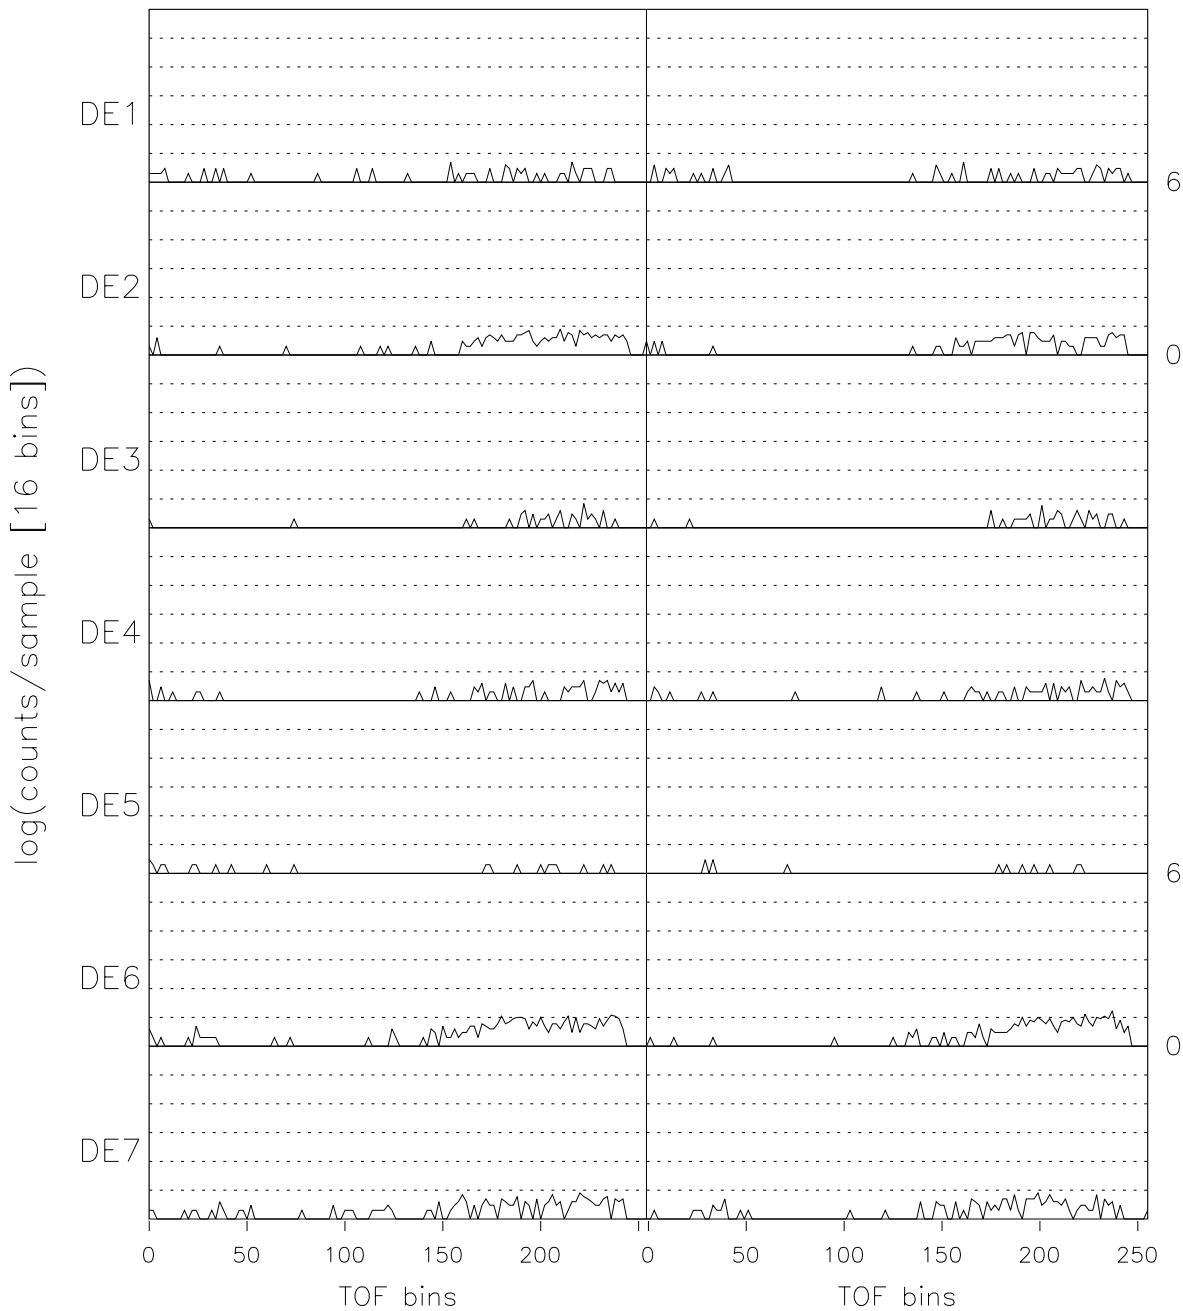

reported: 10-28-06 09:42:40 UT

reported: 10-28-06 09:45:52 UT

file: /export/data/tide/nrt/06102801.dat

-15kV TOF: -9181 v

-3.6kV MCP: -3364 v

-2.4kV MCP: -1784 v

Input Cur: 310 ma

RPA max: 237 v

Mirror max: 238 v